



HAL
open science

Thermal stability of adsorbents used for gas chromatography in space exploration

Leila Bouchra, Cyril Szopa, A. Buch, David Coscia

► **To cite this version:**

Leila Bouchra, Cyril Szopa, A. Buch, David Coscia. Thermal stability of adsorbents used for gas chromatography in space exploration. *Journal of Chromatography A*, 2021, 1644 (May), pp.462087. 10.1016/j.chroma.2021.462087 . insu-03177972

HAL Id: insu-03177972

<https://insu.hal.science/insu-03177972>

Submitted on 24 Apr 2023

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Distributed under a Creative Commons Attribution - NonCommercial 4.0 International License

1 **Thermal stability of adsorbents used for**
2 **gas chromatography in space exploration**
3

4
5 L. Bouchra¹, C. Szopa^{1,2}, A. Buch³, D. Coscia¹
6

7 ¹Laboratoire Atmosphère, Milieux, Observations Spatiales (LATMOS),
8 LATMOS/IPSL, UVSQ Université Paris-Saclay, Sorbonne Université, CNRS, CNES, 11 Bd
9 d'Alembert, 78280 Guyancourt, France

10
11 ²Institut Universitaire de France, Paris, France
12

13 ³ Laboratoire Génie des Procédés et Matériaux, CentraleSupélec, Gif-sur-Yvette, France
14
15
16

17 Submitted to J. Chrom. A

18 Version #3 (revised)

19 15th March 2021

20 14 Pages, 9 Figures, 4 Tables
21
22
23
24
25
26
27
28
29

30 All correspondence should be addressed to:

31 Pr Cyril SZOPA,

32 LATMOS/OVSQ, 11 boulevard d'Alembert, 78280 Guyancourt

33 E-mail: cyril.szopa@latmos.ipsl.fr

34 Tel : +33 (0)1 80 28 52 89

35 **Abstract**

36 For analytical purpose, thermal desorption is now used in gas chromatographs developed to analyse
37 the chemical composition of planetary environments. Due to technical constraints, the thermal
38 desorption cannot be as finely controlled as in the laboratory resulting in possible thermal alteration
39 of the adsorbents used. For these reasons, the influence of heat on physical and chemical properties
40 of various adsorbents, either used or that could be used in gas chromatographs for space
41 exploration, is studied. If the adsorbents made of carbon molecular sieves and graphitised carbon
42 black that were tested show a very high thermal stability up to 800°C, the porous polymers tested
43 are highly degraded from a minimum temperature that depends on the nature of the polymer. Poly-
44 2,6-diphenylphenylene oxide is shown to be the more thermally robust as it is degraded at higher
45 temperatures, confirming it is currently the best choice for analysing organic molecules with a space
46 instrument. Finally, the products of degradation of the porous polymers tested were analysed after
47 heating the porous polymers at 400°C and 800°C. They were identified and listed as potential
48 contaminants of analyses performed with this type of adsorbent. If the exposure to the higher
49 temperature produces numerous organic compounds, mainly aromatic ones, a few ones are also
50 detected at the lower temperature tested, meaning they should be considered as potential
51 contaminants. Again poly-2,6-diphenylphenylene oxide should be preferred because it releases less
52 organic compounds, the structure of which is completely specific to the adsorbent composition.

53

54 **Highlights**

55 Thermal evolution of adsorbents used for GC in space exploration is studied up to 800°C

56

57 Graphitised carbon blacks and molecular sieves are thermally stable

58

59 Porous polymers are drastically degraded by the heat

60

61 Potential organic contaminants produced by porous polymers are tentatively identified and listed

62

63

64 **Keywords**

65 Gas chromatography

66 Thermal desorption

67 Adsorbents

68 Thermal stability

69 Space exploration

70

71

72 1. Introduction

73 Gas chromatography has been used for decades for space exploration [1]. Due to its robustness and
74 relative technical simplicity, this instrumentation has been part of the scientific payload of several
75 space probes that explored Venus [2], Mars [3, 4], comets [5] and even Titan [6]. It is used for the
76 analysis of the chemical composition of the atmospheres, and of condensed materials collected at
77 the surface or in the atmospheres of these bodies. It is favoured to characterize the molecular
78 composition of complex samples containing, or releasing, numerous gaseous compounds which
79 cannot be directly identified with spectrometry alone (e.g. [7]). Through time, the complexity of
80 space experiments increased to get more and more information from the analysed samples.

81 In particular, the preparation of samples (mainly the solid ones) has become more and more complex
82 for gas chromatography in space exploration, to reach the ambitious scientific goals of the
83 instruments, and to meet the technical constraints imposed by the flight of the space probes and the
84 *in situ* operations. For the last chromatographs we built to explore the surface of Mars, this results in
85 quite long times of transfer from the sampling system to the gas chromatographs. For this reason,
86 our team transposed the thermal desorption technique, commonly used in the laboratory to analyse
87 breath samples [8] or to monitor air composition [9], to space application. During the sampling
88 phase, it allows to trap the maximum amount of analytes (enrichment) and spatially focalize them for
89 the transfer duration. During the injection phase, it allows to transfer the trapped chemical species
90 into the chromatographic columns as fast as possible. The whole process is assumed to ensure to
91 have the best possible separation of the analytes with the best detection sensitivity. We did it first
92 successfully for the Sample Analysis at Mars (SAM) experiment onboard the Curiosity rover currently
93 exploring the Mars surface [3], and we will improve it for future missions, as Exomars 2020 [10].

94 In this frame, adsorbents of different natures are used, depending on the chemical species to be
95 analysed. For example, in SAM, Carbosieve is used to trap the most volatile species and Tenax® (TA
96 and GR) for the other volatile compounds. Some of these adsorbents have an upper temperature of
97 thermal stability quite close to their usual recommended operational temperature (400°C as the limit
98 temperature against about 300 °C for operating Tenax®). Moreover, as on Earth, despite their
99 interest for trapping the analytes, adsorbent can be a source of organic molecules which are finally
100 observed in the chromatograms with the analytes released by the sample (see [11] for an example).
101 Then, the compounds released by the adsorbent can be contaminants of the analysis and it is
102 important to limit their contribution, and to clearly identify them in order to discriminate them from
103 the analytes present in the samples. The knowledge of the nature of these possible contaminants
104 prior to the *in situ* measurement is of high importance because the operation limitations of space
105 instruments usually do not allow to perform systematic blank runs to identify background
106 contributions.

107 Usually, these by-products are produced through thermal decomposition or alteration of the
108 adsorbent. For space exploration, the need for building light, sturdy and relatively simple
109 instruments, added to the fact that environmental conditions of the instrument cannot be perfectly
110 stabilized, results in a much less accurate thermal control of the desorption unit compared to
111 laboratory instrumentation. As a consequence, some adsorbent present in the trap could be
112 submitted to a thermal stress (e.g. maximum temperature overshoot) sufficient to lead to an
113 alteration of the adsorbent. These are the main reasons why we performed a systematic study of the
114 behaviour of various adsorbents of interest for space application, when submitted to temperatures
115 up to 800°C. This article presents observed changes of physical and chemical features of different
116 adsorbents commonly used in analytical chemistry when submitted to thermal stress, and the
117 lessons learned for their use in space instrumentation specifically.

118

119

120 **2. Material and methods**

121 2.1. Adsorbents

122 Three main types of adsorbents are commonly used for thermal desorption injection with gas
 123 chromatography: i. carbon black for organic molecules of low to medium weight; ii. porous polymers
 124 for organic molecules of medium to heavy weights; iii. and molecular sieves rather devoted to small
 125 molecules and noble gases. In this work, we studied these all three types of adsorbent materials
 126 which are listed in Table 1. We studied the all three categories of adsorbents, and we selected at
 127 least two different adsorbents of each type to compare their behaviour when submitted to thermal
 128 treatment.

129 For graphitized carbon blacks (GCB), Carbopack B is the more commonly used today but we also
 130 tested Carbopack C. For porous polymer, Tenax® TA is a critical adsorbent for analysing the trapping
 131 and injection of organic molecules in the experiments developed to explore the surface of Mars [3,
 132 10], and an adsorbent commonly used to monitor the Earth atmosphere composition [12]. This is the
 133 reason why in addition to its nature, we also studied the influence of the size of Tenax® TA particles
 134 on its thermal behaviour. Tenax® GR is a mixture of Tenax® TA and GCB, and it is used for trapping
 135 lower molecular weight compounds. Both Tenax® adsorbents are used in the SAM experiment [3].
 136 Porapak Q is another type of porous polymer that could be used in a gas analyser onboard a future
 137 Russian landing probe to the moon surface named Luna Resours [13]. Finally, among the molecular
 138 sieves, we studied Carbosieve SIII which is also used in the SAM instrument on Mars, and Molsieve
 139 5A which is of different chemical composition and could have an interest for future applications in
 140 space exploration, especially for analysing very volatile organic and inorganic molecules, as well as
 141 noble gases.

Adsorbent commercial name	Type of adsorbent	Density (g.mL ⁻¹)	Specific area (m ² .g ⁻¹)	Particle size (mesh)	Maximum operating temperature (°C)
Carbopack C	Graphitized carbon black	0.64	10	80-100	400
Carbopack B	Graphitized carbon black	0.38	100	60-80	400
Tenax® TA	Porous polymer	0.25	35	60-80	350
Tenax® TA	Porous polymer	0.29	35	80-100	350
Tenax® GR	Porous polymer	0.40	25	n.a.***	350
Porapak Q	Porous polymer	0.66	550	50-80	250
Carbosieve SIII*	Molecular sieve	0.72	975	n.a.	400
Molsieve 5A**	Molecular sieve	0.34	n.a.	80-120	300

142 *Table 1: Adsorbents used in this study and their main characteristics. Data from suppliers (Supelco, Sigma-Aldrich).*

143 **Carbosieve SIII is a graphitized carbon black but its specific area makes places it in the molecular sieves category;*

144 ***Molsieve 5A is a zeolite carbon molecular sieve; ***Not available.*

145 2.2. Scanning Electron Microscopy

146 In order to physically characterize each adsorbent studied and their possible evolution when
 147 submitted to pyrolytic conditions, Scanning Electron Microscopy (SEM) was used. With this aim, a
 148 few particles of each adsorbent, either taken from their original vial, or collected in the pyrolysis cup
 149 after their heating, have been deposited on a double-sided tape composed of carbon to ensure the

150 electric conduction required for performing SEM measurements. The adsorbents were analysed in
151 low vacuum mode at a 0.45 torr pressure with an acceleration voltage of 15 kV. The particles of
152 adsorbent were observed in an Environmental Scanning Electron Microscope (ESEM FEI Quanta 200).

153 2.3. Thermal Gravimetry Analysis and Evolved Gas Analysis

154 Thermal evolution study of most of the adsorbents selected were carried out using Thermal
155 Gravimetry Analysis (TGA). Among the thermal analysis techniques, TGA is commonly used for
156 characterizing the thermal properties of both inorganic and organic materials. It allows to measure
157 the sample mass loss as a function of the sample temperature and time. TGA analyses were
158 performed using a SENSYS evo (Setaram) TGA instrument, using a CALISTO software for data
159 recording and treatment. The samples were placed in a 100 μ L platinum crucible. The average
160 sample mass put in the crucible was approximately 20 mg for each analysis. The samples were
161 heated from the ambient temperature ($\sim 20^\circ\text{C}$) to 1000°C at a $10^\circ\text{C}\cdot\text{min}^{-1}$ heating rate and in an argon
162 (chemically inert) atmosphere to prevent any reactivity of the sample with the carrier gas. Once the
163 maximum temperature was reached, the samples were kept for one hour at the final pyrolysis
164 temperature.

165 In complement to TGA, Evolved Gas Analyses (EGA) were performed to follow the chemical species
166 released by the adsorbents as a function of temperature throughout their heating. With this aim we
167 used an EGA/PY-3030D micro-oven pyrolyser (Frontier Lab), installed on the split/splitless injector of
168 a gas chromatograph (GC/Trace GC Ultra, Thermo Scientific) coupled to a quadrupole mass
169 spectrometer (MS/ISQ LT, Thermo Scientific). A short-deactivated (Siltek™ process of silicon layer
170 deposition, Restek) tube (2.5 m long, 0.10 mm internal diameter) made of stainless steel was
171 installed between the injector and the MS. This geometry is used to ensure a fast transfer of the
172 sample from the injector to the MS, and thus making the correlation between the sample
173 temperature and the volatile species detected with MS easy. Moreover, the gas flow restriction
174 induced by the capillary tube allows to maintain the pressure in the MS sufficiently low to operate it.
175 The main operating conditions of the GC-MS instrument were set as follows: the injector was used in
176 the split mode at a temperature of 250°C ; the column temperature was kept at 250°C and the carrier
177 gas (Helium, 99.9999% purity, Air Liquide) flow rate was set constant to $0.5\text{ mL}\cdot\text{min}^{-1}$ with a split flow
178 rate of $10\text{ mL}\cdot\text{min}^{-1}$. The GC to MS transfer line was heated at 250°C as the electron ionization ion
179 source. The ionization energy was 70 eV and the ions produced were scanned in the 12 to 650 m/z
180 range.

181 For pyrolysis, we applied the following program of temperature to all the adsorbents: 280°C for 30
182 min, then heating at $10^\circ\text{C}\cdot\text{min}^{-1}$ up to 800°C that was maintained for 5 min. The total time of the
183 sequence was 82 min during which the mass spectrometer recorded the signal. Knowing the program
184 of temperature of the pyrolyser as a function of time, the EGA curves representing the MS response
185 as a function of the sample temperature can have been simply obtained by converting the time of
186 analysis in temperature. A mass of 5.0 ± 0.1 mg of each adsorbent was pyrolyzed. It was chosen as a
187 trade-off between the sensitivity of the method and the saturation of the MS signal.

188 2.4. Gas Chromatography-Mass Spectrometry analysis of the products of decomposition of the 189 adsorbents 190

191 The goal of this measurement is the identification of the products of degradation of the
192 adsorbents, if they exist, as they can be possible contaminants in the chromatograms. With this aim,
193 the same experimental set-up as described for the EGA measurements was used. Only the
194 deactivated tube was replaced by a MXT-5 (Restek) chromatographic column with the following

195 geometry: 30 m long, 0.25 mm internal diameter and 0.25 μm stationary phase film thickness. This is
 196 a metallic column (Siltek™ process) with a stationary phase made of poly diphenyl (5%) dimethyl
 197 (95%) siloxane bonded to the deactivated inner wall of the column. The operating conditions were
 198 similar except the flow rate that was set to 1.0 mL.min⁻¹ constant, and the program of temperature
 199 was 35°C for 2 min then heating at 10°C.min⁻¹ up to 300°C maintained for 3 min. The MS was used in
 200 the full scan mode to detect all the ions in the 10-450 m/z range. The mass spectrum of the chemical
 201 species detected were compared to those of the National Institute of Standards and Technology
 202 (NIST) reference mass spectra library for identification. The less retained compounds (up to about 20
 203 min retention) are identified with a significant degree of confidence. The more retained compounds
 204 have a more complex structure and usually a lower signal to noise ratio that increase the uncertainty
 205 of the mass spectra. The identification of the corresponding chemical species can be considered as
 206 essentially tentative. But the chemical structures given should be quite similar to the detected
 207 molecule's one.

208 As the adsorbents are heated too slowly to perform a brief injection of the gases released into
 209 the chromatographic column, a cryofocusing system (Frontier) was used to cool down the head of
 210 the column at the liquid dinitrogen temperature throughout the pyrolysis, and then to inject the
 211 species condensed in a small volume by stopping the cryocooling and heating the column. For each
 212 adsorbent studied, a specific program of temperature was used for pyrolysis. The different pyrolysis
 213 steps are summarized in Table 2 for each adsorbent. After each step, the molecular species released
 214 after reaching the final temperature were analysed with GC-MS. Prior to perform the pyrolysis itself,
 215 a first step consisted in desorbing the species trapped on the adsorbent by heating them at 280°C for
 216 20 min, temperature to which the tested adsorbents are not decomposed, as observed on the EGA
 217 and TGA analyses (even if Porapak Q could be slightly degraded), and because 280°C is very close to
 218 the upper temperatures (300-350°C) usually used to clean the adsorbents in order to limit the
 219 possible contamination [14-16].

220 For this study, we focused only on the main materials that were observed to decompose
 221 thermally, meaning Tenax® TA (60-80 mesh) and Porapak Q. Figure 1 shows the chemical structure of
 222 these two organic polymers. Tenax® GR was not studied as it is composed in part of Tenax® TA which
 223 is the source of the mass loss observed using TGA. 5.0±0.1 mg of material was introduced in the
 224 pyrolyser for Tenax® TA (60-80 mesh) and Carbosieve SIII, and 1.0±0.1 mg of material for Porapak Q.
 225

Adsorbent	Initial temperature	First pyrolysis step	Second pyrolysis step
Carbosieve SIII	80°C (5 min)	10°C.min ⁻¹ up to 300°C (5 min)	10°C.min ⁻¹ up to 800°C (3 min)
Tenax® TA (60-80 mesh)	280°C (5 min)	10°C.min ⁻¹ up to 400°C (3 min)	10°C.min ⁻¹ up to 800°C (3 min)
Porapak Q	280°C (5 min)	10°C.min ⁻¹ up to 400°C (5 min)	10°C.min ⁻¹ up to 800°C (3 min)

226 *Table 2 : Pyrolysis steps used to characterize the nature of the molecules released by the adsorbents when they decompose*
 227 *into volatile molecules. For Tenax® TA and Porapak™ Q were first heated at 280°C for desorbing the species trapped on the*
 228 *adsorbents, before starting the pyrolysis.*

229 3. Results and discussion

230

231 3.1. Thermal decomposition

232

233 TGA analysis

234

235 The use of TGA allowed to follow the mass loss of each sample of adsorbent as a function of the
 236 temperature. The results obtained for all the tested adsorbents are presented in Figure 2.

237 On Figure 2, we can observe two general trends. First, there are adsorbents keeping their
 238 mass almost constant up to 1000°C, the maximum temperature. This behaviour is representative of
 239 materials which are very stable to the temperature. The corresponding adsorbents are the molecular

240 sieves and the graphitized carbon blacks. The mass loss observed at the lowest temperatures (from
241 the ambient to $\approx 200^{\circ}\text{C}$) for Molsieve 5A is attributed to the desorption of atmospheric gases which
242 are efficiently trapped by this material. It is not observed for the carbon molecular sieves tested
243 which are not efficient to trap these low mass species (see [17] as an example for an application to
244 space science). This is not fully surprising to observe such a stability as the materials produced to
245 make these adsorbents are usually obtained by controlled pyrolytic processes occurring usually at
246 temperatures up to $700\text{--}800^{\circ}\text{C}$. Now, when looking more carefully at the curves, we observe a small
247 loss of mass for these materials ($\approx 4\%$ for Carbopack B, $\approx 5\%$ for Carbosieve SIII, and $\approx 2\%$ for Molsieve
248 5A), the loss occurring rather at the highest temperatures (typically above 800°C). This indicates a
249 very limited decomposition that should impact the superficial part of the adsorbent only or this could
250 be ascribed to moisture vaporization [18, 19].

251 Then, we observe that the adsorbents made of porous polymers are resistant to the increase of
252 temperature up to a threshold temperature for which they are subjects to a significant mass loss of
253 tens of percent. This corresponds to a massive thermal decomposition that should be accompanied
254 by an outgassing of volatile molecules. Once this large mass loss is finished, we observe at the higher
255 temperatures that the adsorbents still lose mass but at a much lower rate. It is interesting to notice
256 that the massive mass loss is observed at the same temperature for Tenax[®] TA and Tenax[®] GR, as the
257 material decomposing for both adsorbents is the same, *i.e.* Tenax[®] TA. It shows that the presence of
258 graphitized carbon black in Tenax[®] GR does not catalyse the thermal decomposition of Tenax[®] TA.
259 Moreover, the mass loss of Tenax[®] GR ($\approx 45\%$) is about 30% less important than for Tenax[®] TA ($\approx 55\%$)
260 as there is only 70%wt of Tenax[®] TA in Tenax[®] GR. The results obtained are therefore consistent with
261 the composition of Tenax[®] GR. For Porapak Q, we observe that the temperature of massive mass loss
262 is lower than for Tenax[®] TA (450°C instead of 550°C), in a range of temperatures similar to those
263 observed in previous studies [20], and that the mass loss is much more significant ($\approx 80\%$). As for
264 Tenax[®], after the massive mass loss, Porapak Q continues to lose mass but at a much lower rate,
265 down to $\approx 95\%$. These observations demonstrate that Porapak Q is made of a material much more
266 fragile to the heat than Tenax[®] TA.

267
268

269 Evolved Gas Analysis

270 On Figure 3 is plotted the evolution of total ion current of the mass spectrometer detector as a
271 function of the temperature for each adsorbent. All the adsorbents were submitted to this
272 diagnostic. Two main behaviours are observed.

273 First, all the adsorbents based on porous polymers show a significant outgassing observed
274 when MS detector response significantly increase. For all three Tenax[®] adsorbents tested, this
275 outgassing is observed from about 475°C to 800°C with a maximum observed at 570°C . The major
276 part of the gases are shown to be released from 475°C to 677°C . The major ion observed throughout
277 the outgassing has $m/z=246$, which is typical of the m/z value of the ion formed from 2,6-diphenyl-*p*-
278 phenylene oxide which is the monomer of the material composing Tenax[®]. For Porapak Q, the
279 outgassing occurs at lower temperatures, basically from 300°C to about 750°C with a maximum gas
280 release observed around 450°C . The major ions observed throughout the outgassing have $m/z=117$
281 and 132. These m/z values are typical from methylstyrene and ethylstyrene ions respectively. The
282 peak observed is broader than those observed for Tenax[®] and most of the outgassing occurs from
283 350°C to 600°C . This may be due to the fact that Porapak Q is made of a copolymer of
284 ethylvinylbenzene/divinylbenzene, making its decomposition slower than for pure 2,6-diphenyl-*p*-
285 phenylene oxide polymer. Therefore, it can be concluded that porous polymers are not chemically
286 stable when heated up to 800°C , resulting in a probable loss of their adsorption properties and a
287 possible contamination of the analytical set up with the gaseous molecular species produced if the
288 minimum temperature at which they decompose is reached. As Porapak Q releases gases at lower

289 temperature than Tenax[®], it means it is more fragile when submitted to thermal stress. This explains
290 why its maximum operating temperature recommended by the suppliers is much lower for Porapak
291 Q compared to Tenax[®] (Table 1). It can be noticed that these maximum operating temperatures are
292 effectively lower than the minimum temperatures at which the porous polymers start to release
293 gases. It must also be underlined that results obtained with EGA are in agreement with the TGA
294 measurements.

295 Now focusing on the different Tenax[®] adsorbents studied, we observe that the outgassing is
296 similar for both adsorbents. The only difference observed is the peak area with more material
297 outgassed for Tenax[®] TA (60-80 mesh) and the less observed for Tenax[®] GR. As the mass of
298 adsorbent sampled is the same, it means there are chemical differences that should explain this
299 observation. As said for interpreting TGA data, Tenax[®] GR contains 70% of Tenax[®] TA and 30% of
300 graphitized carbon black, this last adsorbent being stable with the temperature. It thus results that
301 the Tenax[®] GR sample has 30% less material that can decompose compared to pure Tenax[®] TA and
302 this explains why the amount of gases observed to be released by Tenax[®] GR is the lowest one, the
303 corresponding peak area being $\approx 77\%$ of the pure Tenax[®] TA peak area. Concerning the two pure
304 Tenax[®] TA samples, we observe that the adsorbent with bigger particles (60-80 mesh) releases more
305 gases than the adsorbent with smaller particles (80-100 mesh). It thus indicates that there is a
306 particle size effect in the release of products of degradation and bigger particles are more subject to
307 decompose than smaller ones.

308 On Figure 3, the second behaviour observed is an absence of gases released by the molecular
309 sieves and graphitized carbon blacks, whatever the temperature is. This confirms the results
310 obtained with TGA that shows that these adsorbents are all thermally stable up to 800°C. The only
311 exception to this rule is Carbpac C which shows a low outgassing around 550°C (major ions
312 observed have $m/z=91$, 105 and 119, typical from alkylated aromatic species as toluene, or
313 dimethylbenzene). This degassing may be due to the fact that the surface area is smaller for this
314 adsorbent than for the other two.

315 316 3.2. Evolution of the adsorbent grains morphology

317 As we demonstrated the heating of adsorbents up to 800°C could have a significant effect on
318 adsorbents, we tried to follow the physical evolution of the adsorbent particles with temperature.
319 We limited this approach to Porapak Q, Tenax[®] TA and Carbosieve SIII as they are representative of
320 the main behaviour observed for adsorbent to thermal stress and described above.

321 Figure 4 shows images obtained before and after heating Porapak Q adsorbent particles up to
322 800°C. It can be observed that the particle size drastically decreased from $\sim 230 \mu\text{m}$ down to $\sim 80 \mu\text{m}$,
323 but the particles keep a roughly spherical shape. This size decrease is compatible with the significant
324 mass loss of material observed both with TGA and EGA measurements. Looking at a given particle,
325 the soft and homogenous spherical shape observed before thermal treatment, changed to a multi-
326 faces carved surface. If we have no information about surface roughness of the particles with SEM,
327 the decrease of the size of the particle should drastically limit its specific surface, and then its
328 adsorption power. As an organic polymer, Porapak Q material should have significantly graphitized at
329 the temperatures used for the pyrolysis, resulting in a modification of the adsorption properties.

330 Figure 5 shows images obtained before and after heating Tenax[®] TA (60-80 mesh) adsorbent
331 particles to 800°C. As for Porapak Q, the particle size drastically decreased by a factor of about 2, but
332 the particles roughly kept their initial shape. This size decrease is compatible with the significant
333 mass loss of material observed with TGA and EGA measurements. Looking at a given particle, the
334 surface globally looks like similar before and after the heating. But looking closer to the surface, it

335 seems that the highly porous and sinuous surface observed initially, was flattened by the thermal
336 stress. This could indicate a decrease of the porosity of the adsorbent which could induce a loss of
337 adsorption efficiency. Similarly, to Porapak Q, the decrease of the size of the particles, and the likely
338 graphitization of the polymer should drastically limit its adsorption properties.

339
340 Figure 6 shows images obtained before and after heating Carbosieve SIII adsorbent particles to
341 800°C. In this case, the particles keep their original size and shape after heating them up to 800°C.
342 This is consistent with the absence of mass loss observed with TGA and EGA measurements. The only
343 change observed is related to the surface roughness of the particles. Indeed, if initially the particle
344 surface is flat and soft, after heating up to 800°C, we observe a fluffier material. This shows that if
345 Carbosieve SIII is globally thermally resistant, its structure is modified by the thermal treatment. And
346 this change should modify its adsorption properties as the manufacturer recommend not to use it at
347 temperatures higher than 400°C (Table 1).

348 349 3.3. Volatile products of degradation

350 The programs of temperatures used to heat the different adsorbents were defined from the
351 results obtained with TGA and EGA analyses. The different ranges of temperature defined
352 correspond to different steps of mass loss from the adsorbents observed with TGA, which may
353 correspond to steps of decomposition releasing different volatile molecules. By sharing the pyrolysis
354 in steps, we wanted to test this assumption.

355 Figure 7 shows the chromatograms obtained when analysing the gases released by Carbosieve
356 SIII after the pyrolysis. It can be observed that only a few compounds are detected. If we except the
357 peaks attributed to column bleeding, only methanol, water and carbon dioxide are detected.
358 Methanol and water are mostly observed at the lowest temperatures the adsorbent is heated,
359 meaning these chemical species should be mainly desorbed from the adsorbent, and that they are
360 not products of decomposition of Carbosieve SIII. Water comes from the atmosphere whereas
361 methanol probably comes from residual solvent used to clean the material used to prepare the
362 sample for pyrolysis. Carbon dioxide is observed on both chromatograms. This is compatible with
363 background CO₂ present in the carrier gas which is trapped by the cold trap. This analysis confirms
364 that Carbosieve SIII does not decompose into volatile species when heated to high temperatures, as
365 already shown by TGA.

366 Figure 8 shows the chromatograms obtained after analysing the products of pyrolysis of Tenax® TA
367 (60-80 mesh) for the two steps of the pyrolysis it was submitted to. Most of the chemical species
368 identified in these chromatograms are listed in Table 3.

369 For the lower pyrolysis temperatures range (from 280 to 400°C), water and carbon dioxide mainly
370 coming from the air present in the background of the carrier gas are detected. In addition to
371 products of decomposition of the column's stationary phase, a few polyaromatic compounds are
372 observed late in the chromatogram. These polyaromatic molecules tentatively identified from their
373 mass spectra, have a structure which is compatible with products of degradation from Tenax® TA
374 because they include aromatic and cyclic structures that bear oxygen atoms. In spite of the detection
375 of these degradation products, we can notice that they are limited in number, and that they have a
376 really characteristic molecular structure compared to usual organic molecules targeted by the
377 chromatographs used for space exploration. This demonstrates that Tenax® TA is quite thermally
378 stable up to 400°C, confirming the observations done with TGA and EGA analyses. This also in
379 accordance with the maximum recommended operating temperature given by the supplier (350°C),
380 which should be the temperature around which these compounds should start to be released by
381 Tenax® TA.

382 For the higher pyrolysis temperature range (Figure 8b), numerous organic compounds are detected
 383 in addition to air and products of degradation of the column stationary phase (Table 3). Most of
 384 these compounds are monoaromatic or polyaromatic compounds bearing oxygen or not. The two
 385 compounds the more retained detected after the low range of temperature pyrolysis are not present
 386 in this chromatogram. This is likely due to the higher temperatures used in this case that should
 387 prevent the formation of these species, or that could degrade them in lighter ones. The most
 388 abundant compounds detected in the chromatogram is the alcohol derived from 2,6-diphenyl-p-
 389 phenylene oxide (peak #14 in Figure b). This observation is in agreement with the TGA
 390 measurements. But many other molecules are observed in various abundances, with molecular
 391 structures which can be easily derived from the decomposition or rearrangement of 2,6-
 392 diphenylphenylene oxide. Then, the detected molecules must be released by Tenax® TA. This
 393 experiment shows the dramatic effect of heating Tenax® TA at temperatures higher than 400°C
 394 because the number and the amount of degradation compounds produced is significant. In addition
 395 to the certain alteration of its adsorption properties, this result shows that this adsorbent must not
 396 be heated at temperatures higher than 400°C because it can produce numerous organic molecules
 397 that can interfere with the detection and identification of molecules present in the analysed sample.
 398 Indeed, many of the degradation products detected (like benzene or phenol) are not strictly
 399 characteristic of the adsorbent because these chemical species can be found in many environments,
 400 including planetary ones [21]. Then their presence in the chromatograms measured *in situ* would
 401 lead to confusing situations for the identification of molecules indigenous to the probed
 402 environment.

403 As a conclusion, this study shows that Tenax® TA is quite stable when heated up to about 400°C,
 404 releasing only a low amount of polyaromatic molecules very specific to the polymer, but Tenax® TA is
 405 significantly degraded when heating it up 800°C, leading to the massive release of numerous
 406 molecules susceptible to contaminate the analysis.

280-400°C first pyrolysis step (desorption)		400-800°C second pyrolysis step (degradation)	
Retention time (min)	Compounds name	Retention time (min)	Identified compounds name
3.1	¹ CO ₂	3.3	¹ CO ₂
3.7	² H ₂ O	5.0/B ^a	² H ₂ O
13.7	*Stationary phase fragment	6.8/B	³ benzene
18.4	Stationary phase fragment	11.4/B	⁴ toluene
21.2	Stationary phase fragment	13.8	*Stationary phase fragment
23.7	Stationary phase fragment	15.2	⁵ ethylbenzene
26.0	Stationary phase fragment	15.7	ethynylbenzene
28.0	Stationary phase fragment	16.2	⁶ styrene
29.5	<i>1,1,3,3 tetramethylbutyl phen-2-ol^b</i>	17.0	methylethyl-benzene isomer
34.4	<i>m-tertphenyl-2-ol</i>	17.6	propenylbenzene
40.3/B	³ not identified	17.8	propylbenzene
49.3/B	⁴ not identified	18.2	benzaldehyde
		18.4	*Stationary phase fragment
		18.5	phenol
		18.6	propenyl-2-benzene
		18.9	benzofuran

		19.4	ethenylmethylbenzene isomer
		19.6	ethenylmethylbenzene isomer
		19.8	propynylbenzene isomer
		19.9	methylphenol isomer
		20.2	acetophenone
		20.9	methylbenzofuran isomer
		21.2	*Stationary phase fragment
		21.7	methylindene isomer
		21.8	<i>4-methylbenzylvinylether</i>
		21.9	methylindene isomer
		22.3	⁷ Naphtalene
		22.7	3-phenyl-3buten-2-one
		22.8	<i>2,3 dihydro-3-methyl Inden-1-one</i>
		23.7	*Stationary phase fragment
		23.9	methyl naphthalene isomer
		24.3	methyl naphthalene isomer
		25.0	<i>4-phenyl 3-butene-2-one</i>
		25.3/B	⁸ biphenyl
		25.8	diphenylmethane
		26.6	methylbiphenyl isomer
		26.7	methylbiphenyl isomer
		27.1	⁹ hydroxybiphenyl isomer
		27.2	<i>dibenzofuran</i>
		27.9	<i>methylphenylphenol isomer</i>
		27.95	<i>phenalene isomer</i>
		28.0	<i>4-phenyl-4-cyclopentene-1,3-dione</i>
		28.2	<i>methylphenylphenol isomer</i>
		29.3/B	¹⁰ hydroxybiphenyl
		30.3	phenanthrene
		30.8	¹¹ biphenyldiol isomer
		30.9	<i>9-vinylanthracene</i>
		31.0	<i>2-dibenzofuranol</i>
		31.1	terphenyl isomer
		32.2	¹² phenylnaphtalene isomer
		33.7	phenylmethyl naphthalene isomer
		33.9/B	¹³ tertphenyl isomer
		35.3/B	¹⁴ <i>m-tertphenyl-2-ol</i>
		35.6	phenyldibenzofuran isomer
		35.7	¹⁵ phenyldibenzofuran isomer
		37.5/B	¹⁶ <i>tertphenylol isomer</i>
		38.1/B	¹⁷ <i>4,4 hydroxyphenoxybiphenyl</i>
		38.8/B	¹⁸ not identified
		39.4	<i>9-phenyl-9-fluorenl</i>
		41.4	terphenyl-phenyl isomer
		42.1	<i>4-triphenylmethylphenol</i>

		43.3	<i>Triphenylphenol msse 322 proeminente</i>
		44.4	<i>Triphenylphenol</i>
		48.6	<i>Triphenylphenol</i>
		50.6	<i>Triphenylphenol</i>

407 *Table 3 : Retention time and name of each compound released by Tenax® TA (60-80 mesh) after each heating step applied*
408 *to the adsorbent. Indices refer to the peak attribution given in Figure 8. ^aB is indicated when the corresponding peak is broad*
409 *in the chromatogram. ^bChemical species written in italics are tentatively identified only, with NIST match score typically*
410 *below 800.*

411 Figure 9 shows the chromatograms obtained after analysing the products of pyrolysis of Porapak Q
412 for the two steps of the pyrolysis it was submitted to. Most of the chemical species identified in
413 these chromatograms are listed in Table 4.

414 For the lower pyrolysis temperatures range (from 280 to 400°C, Figure 9a), water and carbon dioxide
415 mainly coming from the air present in the background of the carrier gas are detected. In addition to
416 products of decomposition of the column's stationary phase, several aromatic and cyclic organic
417 molecules are observed in the chromatogram. The detected molecules are mostly monoaromatic
418 molecules which are either ramified or associated to a cyclic structure (aromatic or not). Such
419 molecular structures are compatible with the pyrolysis of the ethylvinylbenzene-divinylbenzene
420 copolymer that leads to the production of a monoaromatic motifs, combined with products of the
421 alteration or modification of the linear carbon chain of the polymer. Then, for this organic polymer,
422 the number and the amount of compounds released at relatively low temperature is significant.
423 Moreover, the nature of the compounds, even if they are specific to the copolymer, can be difficult
424 to discriminate from organic molecules indigenous to samples that can be analysed in planetary
425 environments, like on Titan that is a medium rich in hydrocarbons (see [22-24] for instance).
426 Therefore, Porapak Q is an adsorbent relatively thermally weak at 400°C, producing several organic
427 molecules that can interfere with the analysis of a sample. This explains why its maximum
428 recommended operating temperature given by the supplier (250°C) is lower than for Tenax® TA.

429 For the higher pyrolysis temperature range (Figure 9b), numerous organic compounds are detected
430 in addition to air and products of degradation of the column stationary phase (Table 4). As for low
431 temperature pyrolysis, the majority of the detected compounds are monoaromatic alkylated
432 hydrocarbons. A few biphenylic hydrocarbons are probably present in the last part of the
433 chromatogram, but the uncertainty in the attribution of the chemical species from comparison with
434 the NIST mass spectra library prevents their strict identification, as numerous peaks in this region of
435 the chromatogram (for retention times longer ~than 30 min). These molecular groups being
436 characteristic from those of ethylvinylbenzene-divinylbenzene, the detected molecules must be
437 released by Porapak Q. As for Tenax® TA, this experiment shows the dramatic effect of heating this
438 adsorbent to temperatures higher than 400°C because the number and the amount of degradation
439 compounds produced is significant. In addition to the certain alteration of its adsorption properties,
440 this result shows that this adsorbent must not be heated at temperatures higher than 400°C because
441 it can produce numerous organic molecules that can interfere with the detection and identification
442 of molecules present in the analysed sample. It can also be noticed that the number of species
443 detected when pyrolyzing Porapak Q to 800°C is significantly higher than for Tenax® TA, showing that
444 ethylvinylbenzene-divinylbenzene can produce a larger variety of molecules compared to 2,6-
445 diphenylphenylene oxide.

446 As a conclusion, this study shows that Porapak Q is relatively unstable when thermally stressed. Its
447 use requires to limit strictly its heating to relatively low temperatures (250°C from the supplier)
448 whether it should start to produce many organic molecules susceptible to contaminate the analysis.

280-400°C first pyrolysis step (desorption)		400-800°C second pyrolysis step (degradation)	
Retention time (min)	Identified compounds name	Retention time (min)	Identified compounds name
3.1	¹ CO ₂	3.2	¹ CO ₂
3.8	² H ₂ O	3.4	butene isomer
13.6	* Stationary phase fragment	4.1/B ^a	² H ₂ O
16.0	³ styrene	5.4	isobutyronitrile
17.9	ethylmethylbenzene isomer	6.2	³ benzene
18.4	Stationary phase fragment	11.1	⁴ toluene
18.7	⁴ propenyl-2-benzene	13.7	* Stationary phase fragment
20.5/B	⁵ ethenylethylbenzene isomer	15.1	ethylbenzene
20,7/B	⁵ ethenylethylbenzene isomer		
21.0	diethenylbenzene isomer	15.5/B	⁵ xylene isomer
21.3	diethenylbenzene isomer	16.3/B	⁶ styrene
21.8	<i>methylbutenylbenzene^b</i>	17.9/B	⁷ ethylmethylbenzene isomer
22.2	⁶ not identified	18.5	* Stationary phase fragment
22.4	not identified	18.9	⁸ propenyl-2-benzene
22.7	not identified	19.4	methylmethylethylbenzene isomer
23.4	<i>ethylphenylethanone isomer</i>	19.8	diethylbenzene isomer
23.7	⁷ phenylbutenone isomer	20.0	diethylbenzene isomer
24.0	<i>phenylbutenone isomer</i>	20.8/B	⁹ ethenylethylbenzene isomer
32.2	not identified	21.4	diethenylbenzene isomer
32.4	not identified	21.5	<i>methylbutenylbenzene</i>
32.6	not identified	21.9	<i>ethenyltrimethylbenzene isomer</i>
		22.1	not identified
		22.2	<i>ethenyltrimethylbenzene isomer</i>
		22.3	not identified
		22.5	¹⁰ not identified
		22.8	<i>ethylindene</i>
		23.1	<i>methyleneethylmethylbenzene isomer</i>
		23.4	<i>ethylmethylethylbenzene isomer</i>
		23.6	<i>bismethylethenylbenzene isomer</i>
		23.8/B	¹¹ phenylbutenone isomer
		24.1/B	¹² phenylbutenone isomer
		24.9	¹³ methylethenylphenylethanone isomer
		25.1	<i>phenylbutenone isomer</i>
		25.2	not attributed
		25.3	<i>methylethenylphenylethanone isomer</i>
		25.4	<i>vinylbenzoic acid isomer</i>
		25.9	biphenyl

		26.5	<i>methylbiphenyl isomer</i>
		27.0	<i>methylbiphenyl isomer</i>
		From 28 to 41	Numerous peaks which cannot be identified from their spectrum. But their spectrum contains ions typical from monoaromatic fragments for most of them
		30.5	<i>bisphenylmethylpropane</i>
		31.0	<i>diphenylpentene</i>

451 *Table 4: Retention time and name for each compound released by Porapak Q after each heating step applied to the*
452 *adsorbent. Indices refer to the peak attribution given in Figure 9. ^aB is indicated when the corresponding peak is broad in the*
453 *chromatogram. ^bChemical species written in italics are tentatively identified only, with NIST match score typically below 800.*

454

455 **4. Conclusion**

456

457 Among the adsorbents used, or that could be potentially used, in the development of instruments for
458 space exploration, this study shows that carbon molecular sieves and graphitized carbon blacks are
459 mechanically and chemically inert materials when submitted to temperatures usually used for
460 thermal desorption (~300°C) and pyrolysis (800°C). Without presuming about the effect of thermal
461 treatment on the adsorption properties of these materials, this result proves that these adsorbents
462 can be used without any risk of contamination or degradation of the analytical system. Concerning
463 the porous polymers tested, both are fragile materials when submitted to temperatures higher than
464 ~300°C but Tenax® TA is more robust as a significant degradation is observed only from 600°C. As
465 these adsorbents have similar adsorption properties, this means that Tenax® TA should be preferred
466 as it is more able to resist to local or global overheats that can occur in space instrumentation.
467 Moreover, Porapak Q produces more organic degradation products than Tenax® TA, which should be
468 difficult to discriminate from analytes because they are mostly common monoaromatic
469 hydrocarbons. Tenax® TA produces volatile degradation products which can be more easily
470 identified due to their specific molecular structure, at least at reasonable temperatures relevant to
471 thermal desorption (~300°C). These results therefore strengthen the choice of adsorbents that were,
472 or are still used for thermal desorption in space instrumentation, and they will be useful for the
473 development of new instruments, and for the interpretation of the data collected in the planetary
474 environments explored.

475

476 **Acknowledgements**

477 The authors acknowledge the funding support of the French national space agency, the Centre
478 National d'Etudes Spatiales (CNES) (μ -GC Research and Technology program grant).

479

480 They also thank Nathalie Ruscassier and Jamila El Bekri from CentraleSupélec, for their help to
481 acquire images with Scanning Electron Microscopy, and TGA measurements.

482

483 **References**

- 484 [1] R. Sternberg, F. Raulin, C. Szopa, A. Buch, C. Vidal-Madjar, GAS CHROMATOGRAPHY | Gas
485 Chromatography in Space Exploration, in: I.D. Wilson (Ed.) Encyclopedia of Separation Science,
486 Academic Press, Oxford, 2007, pp. 1-13.
487 [2] V.I. Oyama, G.C. Carle, F. Woeller, J.B. Pollack, Laboratory Corroboration of the Pioneer Venus Gas
488 Chromatograph Analyses, Science, 205 (1979) 52.
489 [3] P. Mahaffy, C. Webster, M. Cabane, P. Conrad, P. Coll, S. Atreya, R. Arvey, M. Barciniak, M. Benna,
490 L. Bleacher, W. Brinckerhoff, J. Eigenbrode, D. Carignan, M. Cascia, R. Chalmers, J. Dworkin, T. Errigo,
491 P. Everson, H. Franz, R. Farley, S. Feng, G. Frazier, C. Freissinet, D. Glavin, D. Harpold, D. Hawk, V.

492 Holmes, C. Johnson, A. Jones, P. Jordan, J. Kellogg, J. Lewis, E. Lyness, C. Malespin, D. Martin, J.
493 Maurer, A. McAdam, D. McLennan, T. Nolan, M. Noriega, A. Pavlov, B. Prats, E. Raaen, O. Sheinman,
494 D. Sheppard, J. Smith, J. Stern, F. Tan, M. Trainer, D. Ming, R. Morris, J. Jones, C. Gundersen, A.
495 Steele, J. Wray, O. Botta, L. Leshin, T. Owen, S. Battel, B. Jakosky, H. Manning, S. Squyres, R. Navarro-
496 González, C. McKay, F. Raulin, R. Sternberg, A. Buch, P. Sorensen, R. Kline-Schoder, D. Coscia, C.
497 Szopa, S. Teinturier, C. Baffes, J. Feldman, G. Flesch, S. Forouhar, R. Garcia, D. Keymeulen, S.
498 Woodward, B. Block, K. Arnett, R. Miller, C. Edmonson, S. Gorevan, E. Mumm, The Sample Analysis at
499 Mars Investigation and Instrument Suite, *Space Science Reviews*, 170 (2012) 401-478.
500 [4] D.R. Rushneck, A.V. Diaz, D.W. Howarth, J. Rampacek, K.W. Olson, W.D. Dencker, P. Smith, L.
501 McDavid, A. Tomassian, M. Harris, K. Bulota, K. Biemann, A.L. LaFleur, J.E. Biller, T. Owen, Viking gas
502 chromatograph-mass spectrometer, *Rev. Sci. Instrum.*, 49 (1978) 817-834.
503 [5] F. Goesmann, H. Rosenbauer, R. Roll, C. Szopa, F. Raulin, R. Sternberg, G. Israel, U.J. Meierhenrich,
504 W.H.P. Thiemann, G. Munoz-Caro, COSAC, the cometary sampling and composition experiment on
505 Philae, *Space Science Reviews*, 128 (2007) 257-280.
506 [6] H. Niemann, S.K. Atreya, S.J. Bauer, K. Biemann, B. Block, G.R. Carignan, T.M. Donahue, R.L. Frost,
507 D. Gautier, J.A. Haberman, D. Harpold, D.M. Hunten, G. Israel, J.I. Lunine, K. Mauersberger, T.C.
508 Owen, F. Raulin, J.E. Richards, S.H. Way, The Gas Chromatograph Mass Spectrometer for the Huygens
509 Probe, *Space Science Review*, 104 (2002) 551-590.
510 [7] C. Freissinet, D.P. Glavin, P.R. Mahaffy, K.E. Miller, J.L. Eigenbrode, R.E. Summons, A.E. Brunner, A.
511 Buch, C. Szopa, P.D. Archer, H.B. Franz, S.K. Atreya, W.B. Brinckerhoff, M. Cabane, P. Coll, P.G.
512 Conrad, D.J. Des Marais, J.P. Dworkin, A.G. Fairén, P. François, J.P. Grotzinger, S. Kashyap, I.L. ten
513 Kate, L.A. Leshin, C.A. Malespin, M.G. Martin, F.J. Martin-Torres, A.C. McAdam, D.W. Ming, R.
514 Navarro-González, A.A. Pavlov, B.D. Prats, S.W. Squyres, A. Steele, J.C. Stern, D.Y. Sumner, B. Sutter,
515 M.P. Zorzano, M.S.L.S.T. the, Organic molecules in the Sheepbed Mudstone, Gale Crater, Mars,
516 *Journal of Geophysical Research: Planets*, 120 (2015) 2014JE004737.
517 [8] M. Xu, Z. Tang, Y. Duan, Y. Liu, GC-Based Techniques for Breath Analysis: Current Status,
518 Challenges, and Prospects, *Critical Reviews in Analytical Chemistry*, 46 (2016) 291-304.
519 [9] A. Cecinato, C. Balducci, D. Mastroianni, M. Perilli, Sampling and analytical methods for assessing
520 the levels of organic pollutants in the atmosphere: PAH, phthalates and psychotropic substances: a
521 short review, *Environmental Science and Pollution Research*, 19 (2012) 1915-1926.
522 [10] F. Goesmann, W.B. Brinckerhoff, F. Raulin, W. Goetz, R.M. Danell, S.A. Getty, S. Siljeström, H.
523 Mißbach, H. Steininger, R.D. Arevalo, A. Buch, C. Freissinet, A. Grubisic, U.J. Meierhenrich, V.T.
524 Pinnick, F. Stalport, C. Szopa, J.L. Vago, R. Lindner, M.D. Schulte, J.R. Brucato, D.P. Glavin, N. Grand, X.
525 Li, F.H.W. van Amerom, M.S.T. the, The Mars Organic Molecule Analyzer (MOMA) Instrument:
526 Characterization of Organic Material in Martian Sediments, *Astrobiology*, 17 (2017) 655-685.
527 [11] P. Axel Clausen, P. Wolkoff, Degradation products of Tenax TA formed during sampling and
528 thermal desorption analysis: Indicators of reactive species indoors, *Atmospheric Environment*, 31
529 (1997) 715-725.
530 [12] A. Kumar, I. Viden, Volatile Organic Compounds: Sampling Methods and Their Worldwide Profile
531 in Ambient Air, *Environ Monit Assess*, 131 (2007) 301-321.
532 [13] L. Hofer, P. Wurz, A. Buch, M. Cabane, P. Coll, D. Coscia, M. Gerasimov, D. Lasi, A. Sapgir, C.
533 Szopa, M. Tulej, Prototype of the gas chromatograph–mass spectrometer to investigate volatile
534 species in the lunar soil for the Luna-Resurs mission, *Planetary and Space Science*, 111 (2015) 126-
535 133.
536 [14] A. Sonnette, M. Millet, R. Ocampo, L. Alleman, P. Coddeville, Tenax-TA Spiking Approach of
537 Thermal Desorption Coupled to GC–MSMS for the Quantification of PAHs in Indoor Air and Dust,
538 *Polycyclic Aromatic Compounds*, 37 (2017) 170-177.
539 [15] L. Chu, S. Deng, R. Zhao, J. Deng, X. Kang, Comparison of Adsorption/Desorption of Volatile
540 Organic Compounds (VOCs) on Electrospun Nanofibers with Tenax TA for Potential Application in
541 Sampling, *PLOS ONE*, 11 (2016) e0163388.

- 542 [16] B. Glas, B. Stenberg, H. Stenlund, A.-L. Sunesson, A novel approach to evaluation of adsorbents
543 for sampling indoor volatile organic compounds associated with symptom reports, *Journal of*
544 *Environmental Monitoring*, 10 (2008) 1297-1303.
- 545 [17] S.A. Aseev, M.V. Gerasimov, M.A. Zaitsev, A.G. Sapgir, Analysis of volatile lunar compounds: The
546 study of gas retention time on Carbosieve SIII adsorbent with respect to temperature, *Cosmic*
547 *Research*, 54 (2016) 358-365.
- 548 [18] F. Cataldo, A study on the thermal stability to 1000°C of various carbon allotropes and
549 carbonaceous matter both under nitrogen and in air, *Fullerenes, Nanotubes and Carbon*
550 *Nanostructures*, 10 (2002) 293-311.
- 551 [19] F. Cataldo, A study on the thermal stability of the. photopolymer, the ozopolymer, and the
552 photochlorinated derivative of C60 fullerene, *Fullerene Science and Technology*, 9 (2001) 55-61.
- 553 [20] C.N. Caçaval, V. Neagu, The thermal degradation of copolymers of vinyltoluene and
554 divinylbenzene, *Polymer Degradation and Stability*, 45 (1994) 423-427.
- 555 [21] S. Vinatier, B. Schmitt, B. Bézard, P. Rannou, C. Dauphin, R. de Kok, D.E. Jennings, F.M. Flasar,
556 Study of Titan's fall southern stratospheric polar cloud composition with Cassini/CIRS: Detection of
557 benzene ice, *Icarus*, 310 (2018) 89-104.
- 558 [22] C.M. Anderson, R.E. Samuelson, D. Nna-Mvondo, Organic Ices in Titan's Stratosphere, *Space*
559 *Science Reviews*, 214 (2018) 125.
- 560 [23] M.L. Cable, S.M. Horst, R. Hodyss, P.M. Beauchamp, M.A. Smith, P.A. Willis, Titan Tholins:
561 Simulating Titan Organic Chemistry in the Cassini-Huygens Era, *Chem. Rev.*, 112 (2012) 1882-1909.
- 562 [24] M. Morisson, C. Szopa, N. Carrasco, A. Buch, T. Gautier, Titan's organic aerosols: Molecular
563 composition and structure of laboratory analogues inferred from pyrolysis gas chromatography mass
564 spectrometry analysis, *Icarus*, 277 (2016) 442-454.

565

566

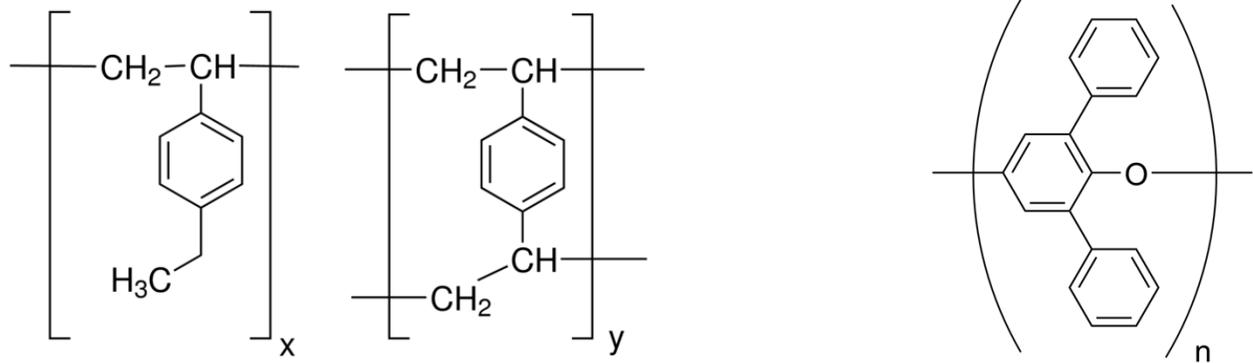


Figure 1

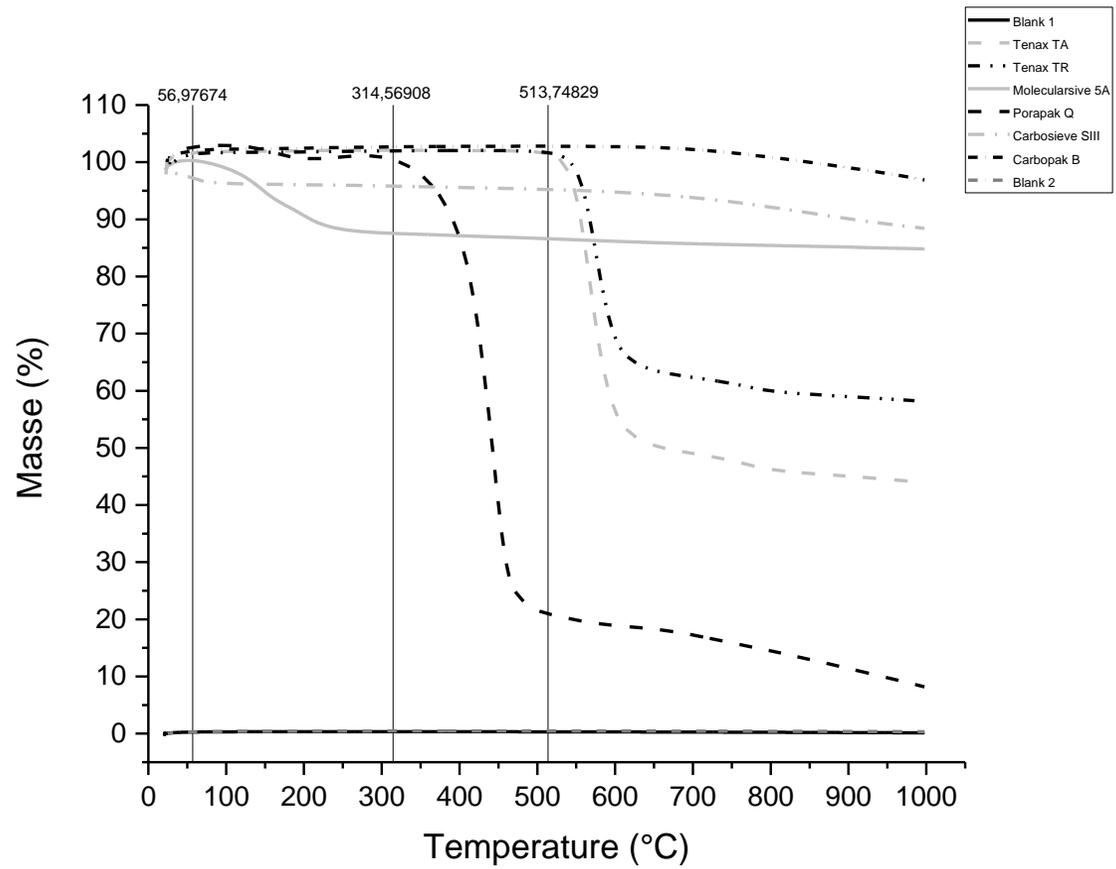


Figure 2

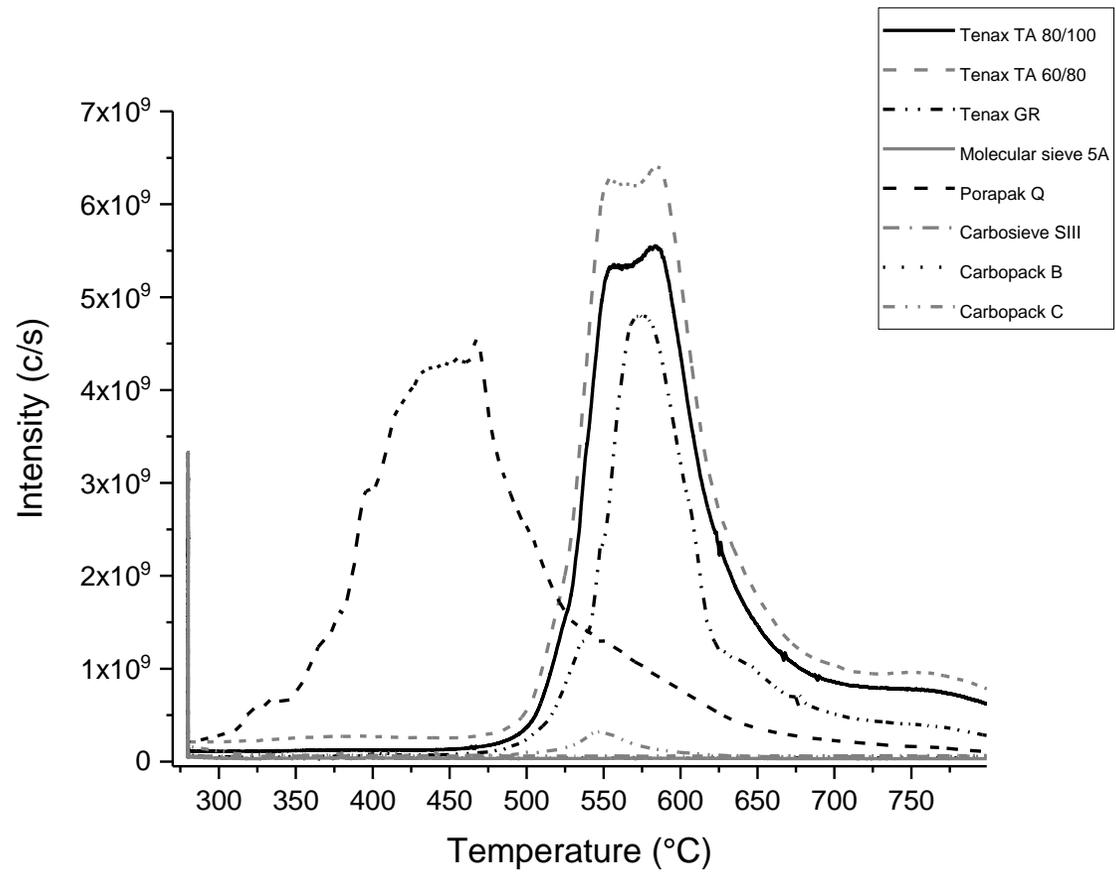


Figure 3

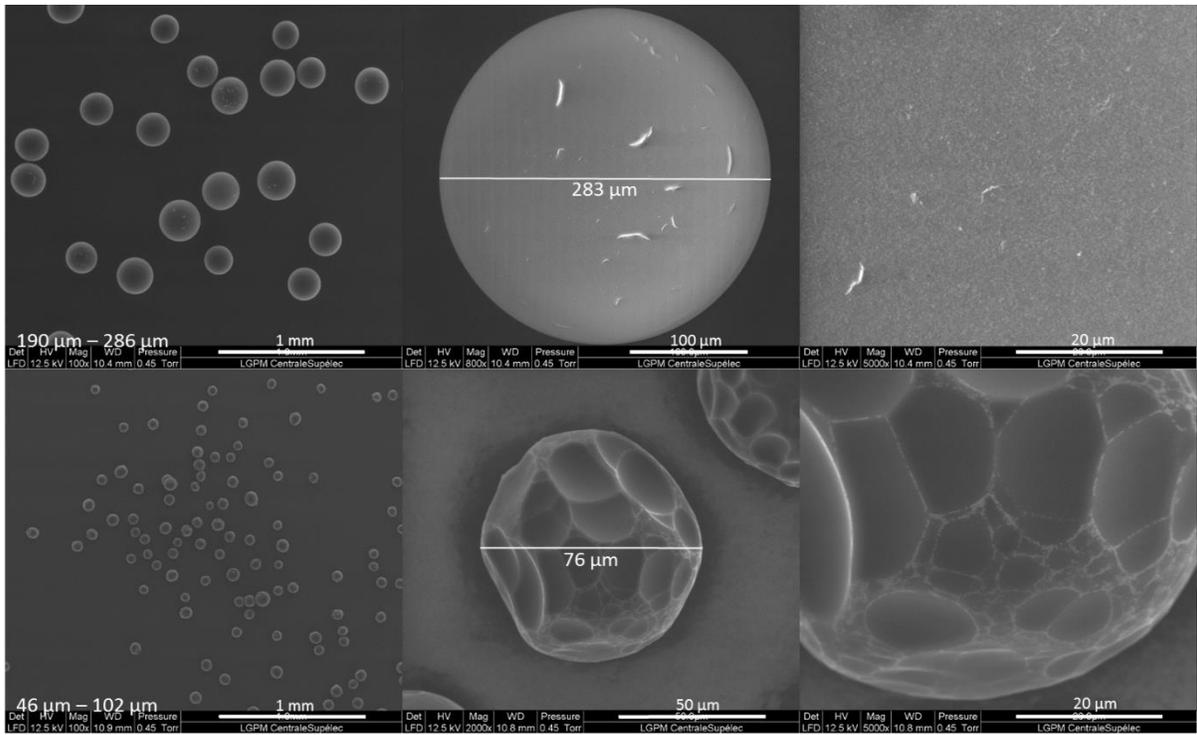


Figure 4

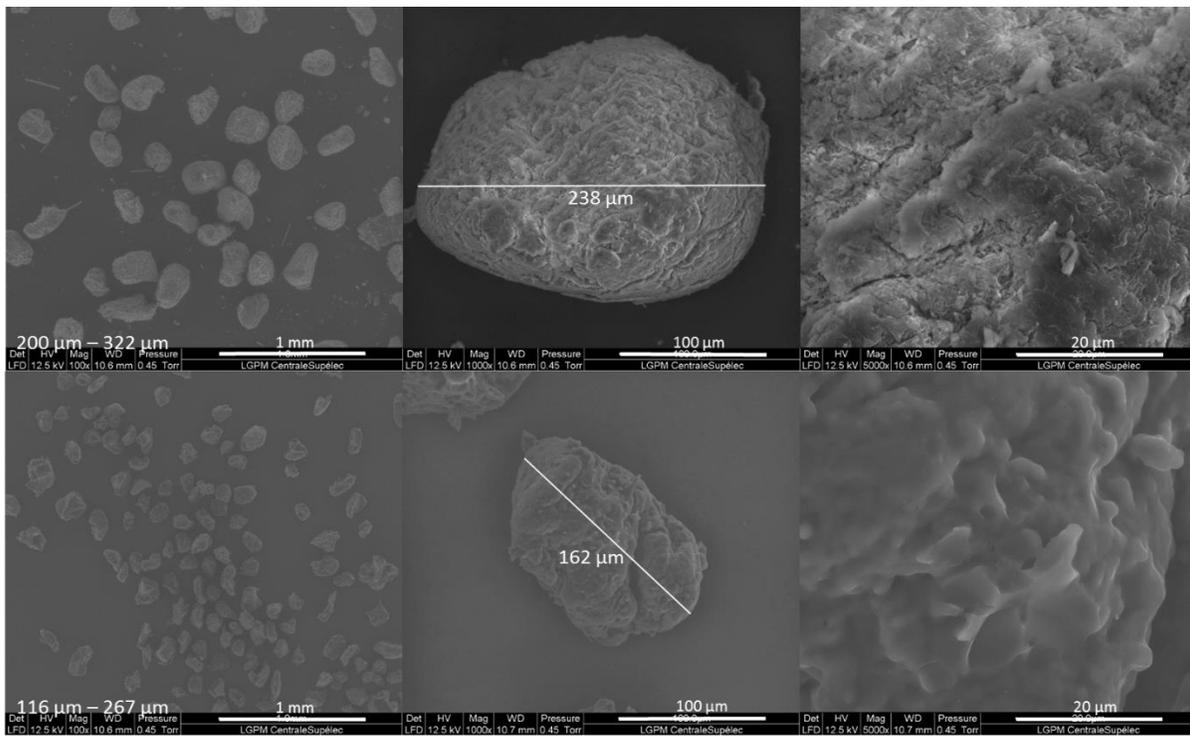


Figure 5

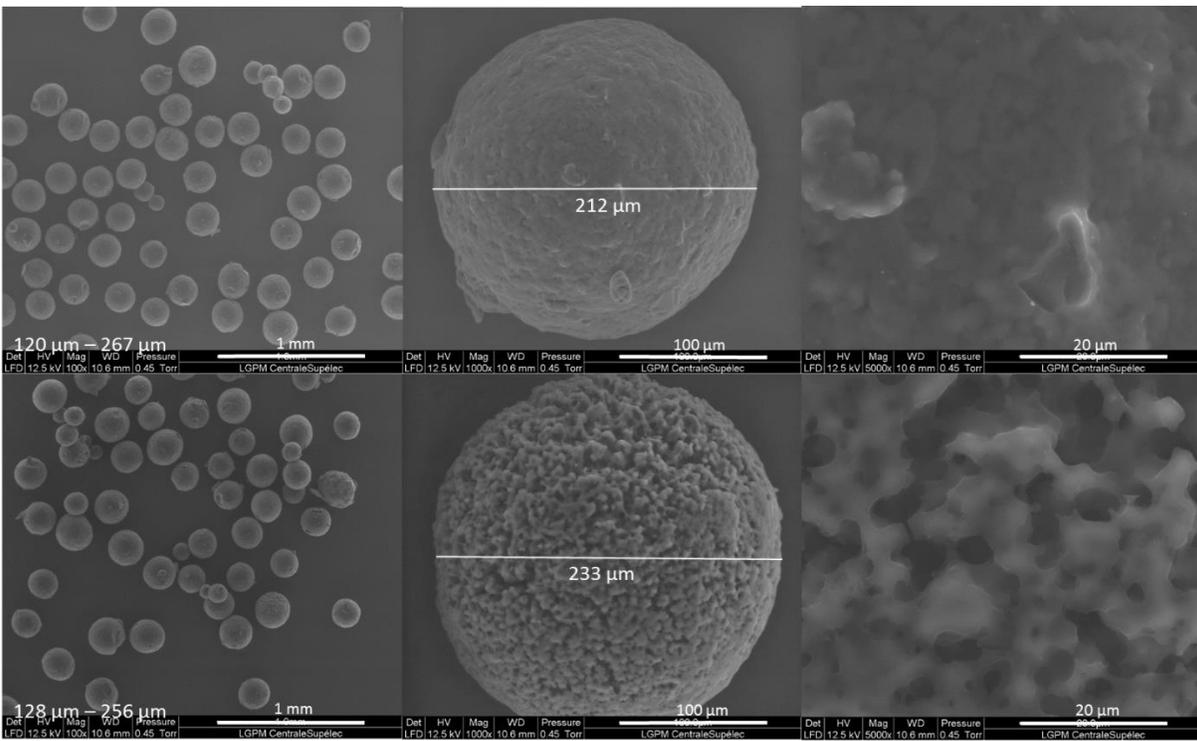


Figure 6

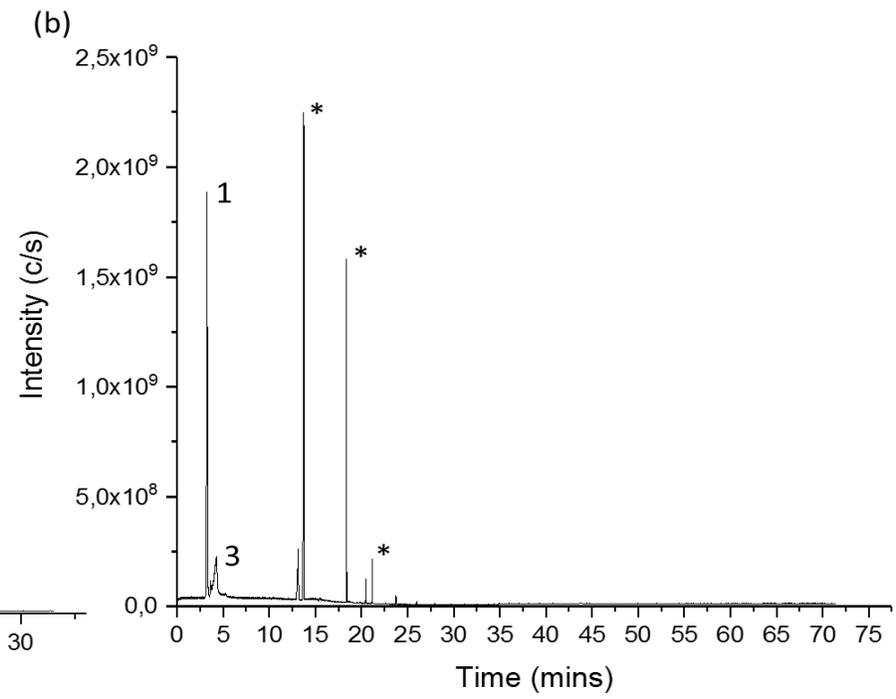
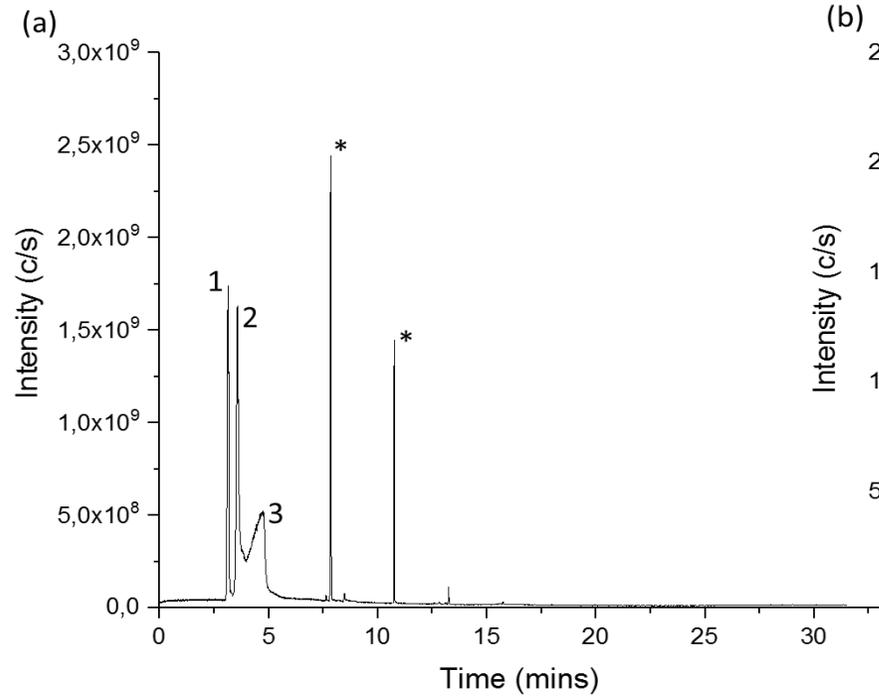


Figure 7

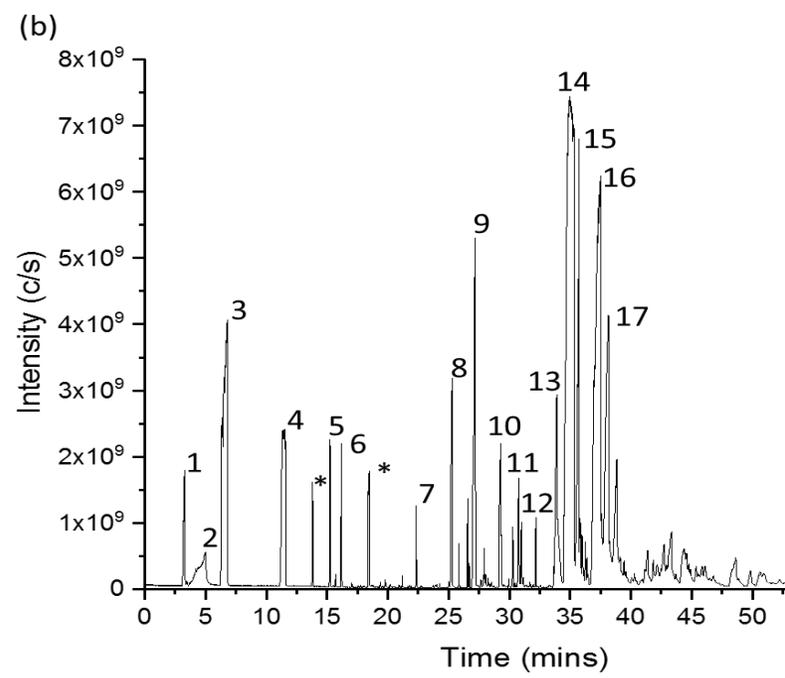
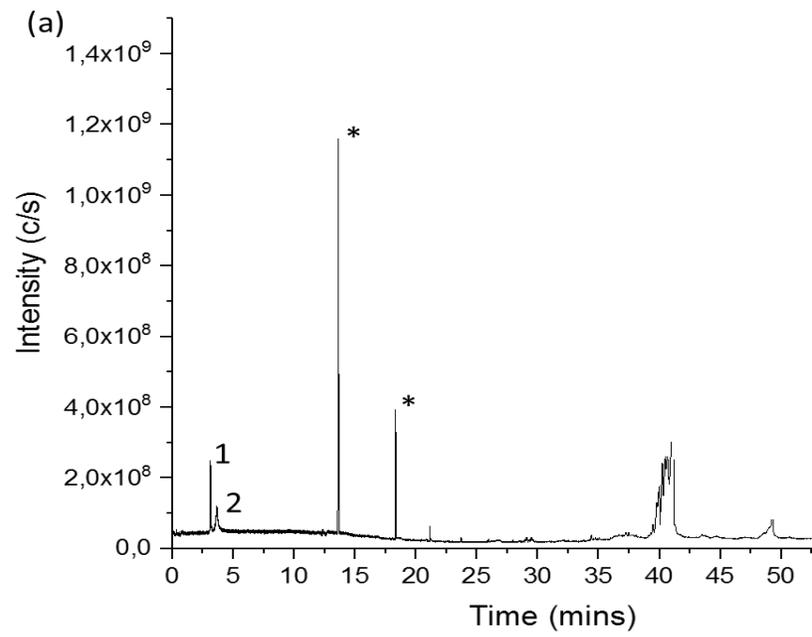


Figure 8

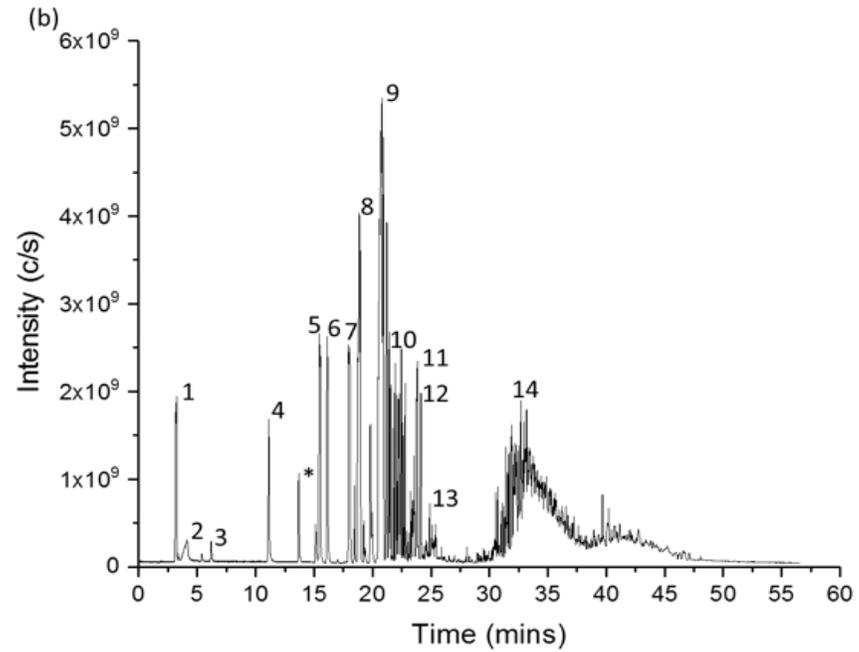
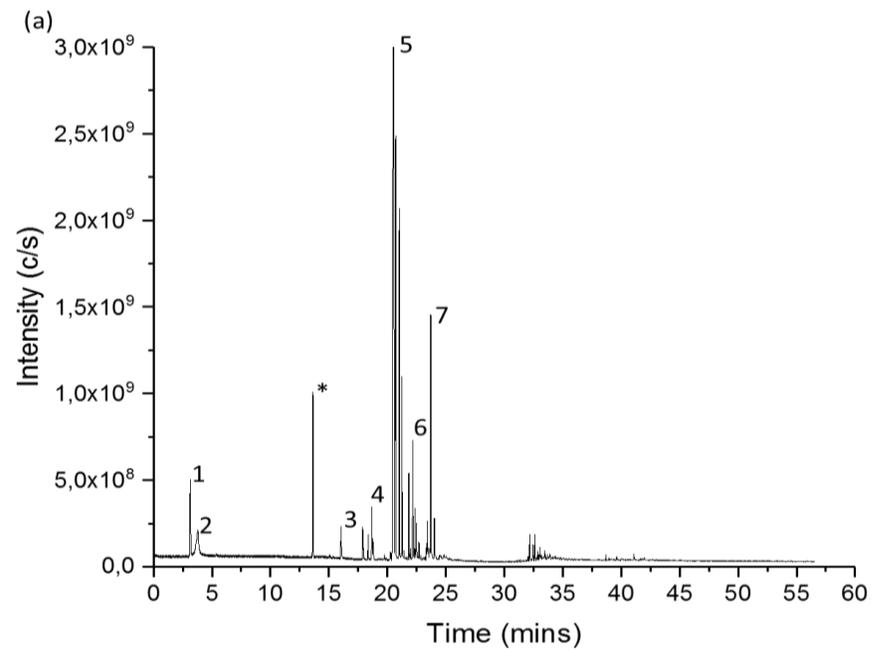


Figure 9